
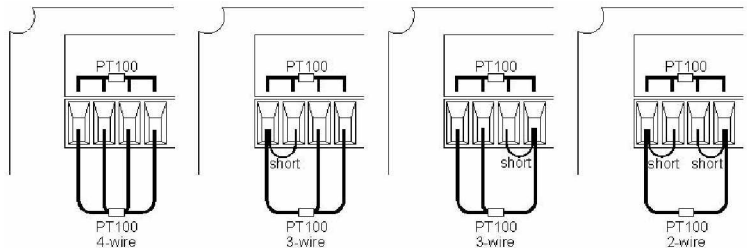


Connection Diagram of Iotron™ Sensors without Preamplifiers to Jenco 6TX 2-Wire pH / ORP Transmitter

Connection from Iotron™ Sensor to Terminal Block on back of Transmitter (READ CAREFULLY)

<u>Cable Color Coding</u>	<u>Sensor Cable Lead Value</u>	<u>Terminal Label As given on Meter</u>	<u>Terminal Value (See Diagram Below)</u>
Black	TC Input	PT100 or 3K, PT1000	ATC IN (No Polarity)
Black	TC Input	PT100 or 3K, PT1000	ATC IN (No Polarity)
Red	Reference Input	pH/ORP (-)	Reference
Clear	pH/ORP Input (Signal)	pH/ORP (+)	pH Glass or ORP

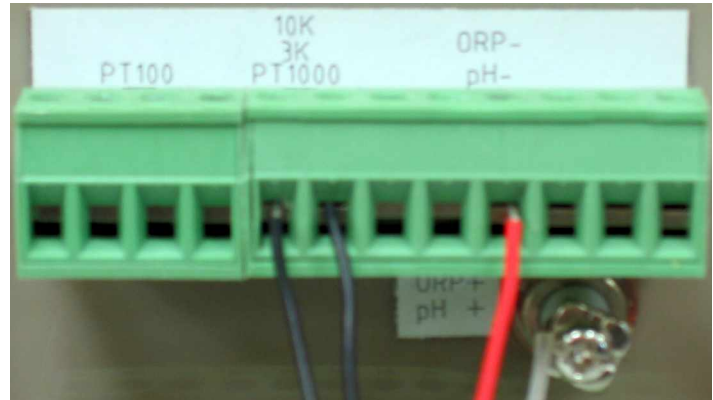

Note: Balco 3K & PT1000 TC elements are only supported as two-wire TC elements.

Special hook-up schematics of 2-wire and 3-wire PT100 temperature compensation (TC) elements to 6TX Transmitters.

Note 1: Automatic Temperature Compensator (ATC) is 3000 Ohm Balco Resistor (-3000-), 1000 (-1000-) or 100 (-100-) Ohm Platinum Temperature Compensation (TC) Element. You must set this TC Value in the Calibration Mode. Use Code: **baLC** for the ATC setting if a 3000 Ohm Balco Resistor is present or use Code: **100 Pt** or **1000 Pt** for the ATC setting if a 100 or 1000 Ohm Platinum TC Element is present (respectively). *If 100 Ohm Platinum TC is used, two jumpers must be employed to support use of 2-wire TC on 4-wire TC input terminal.*

Note 2: The Temperature Compensator element employed can be determined by measuring the resistance between the two black wires on any multimeter (in Ohms).

Note 3: Your first pH buffer value must be 7.00 or 6.86! The second pH buffer value can be 4.01 or 10.00 if starting with pH buffer 7.00 as pH buffer 1. The second pH buffer value can be 4.01 and 9.18 if starting with pH buffer 6.86 as the pH buffer 1. Consult the operation manual for further calibration and power hook-up details.